

## EMDL700

### Environmental Sound/ Temperature and Humidity Datalogger



## ***Introduction***

---

Congratulations on your purchase of the Triplet EMDL700 Environmental Sound/ Temperature and Humidity Datalogger with touchscreen. The EMDL700 measures and records sound levels, temperature, relative humidity, and dew point in real time and displays the readings in digital and graphic formats. The touch-screen menu allows you to program datalogging parameters and to customize the graphic display. Eight (8) GB of memory is included for capturing large amounts of data, easily transferrable to a PC (in CSV format for convenient integration with the most common programs).

## ***Features***

---

- Records up to 20,000 data points
- 7" high-resolution touch screen color LCD display (1024x600)
- Real time graphical curve with zoom and digital display of readings
- Brightness adjustment and screen saver with adjustable start time
- High/Low audible and visual alarms (high alarm only for sound)
- 1 second to 24 hour sampling rate with manual start/stop
- Progress bar indicates used/free memory
- $\pm 1.4$ dB accuracy (IEC61672 -1 Class 2)
- User selectable  $^{\circ}\text{C}/^{\circ}\text{F}$
- Max/Min
- Date and time setting
- USB interface for downloading recorded data to your PC in CSV format
- Built-in desk stand and wall mounting bracket
- Comes complete with sensor probe with 3.3ft (1m) cable, windscreen, USB cable, 3.7V Lithium battery, and AC adapter/charger

## ***Common Applications***

---

- Labs
- Hospitals
- Greenhouses
- HVAC systems
- Office spaces


- Classrooms
- Museums
- Clean rooms
- Calibration labs
- Environmental monitoring
- Health care facilities
- Storage/warehouse monitoring

### ***Meter Description***

---

1. Touch Screen
2. ON/OFF Button
3. Microphone
4. RH Extension Cable
5. Temperature and Humidity Probe/Sensor
6. Support Frame/Tilt Stand
7. Type-C USB Connector



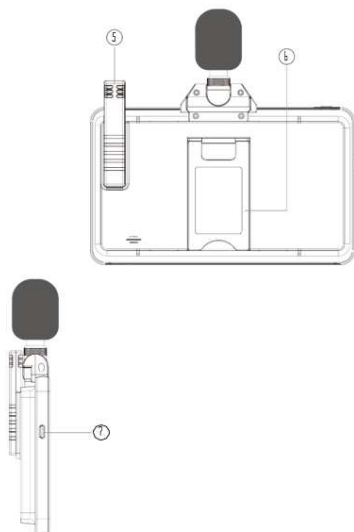

### ***User Interface & Operation***

---

1. Menu function
2. Memory progress bar, “used” indicating used memory, “Free” indicating the remaining memory
3. System real time clock
4. Battery capacity
5. Numerical scale of the temperature, humidity and noise
6. Three curves represent trend of temperature, noise and humidity
7. Numerical scale of date and time
8. Start/Stop recording
9. Max/Min
10. Value of real-time temperature, humidity and noise



The datalogger will automatically give a better HD view in order to watch, when no one is operating it more than 1 minute. As shown below:



- In this picture, it will jump back to the main interface when you touch the screen.

## .Chart Area



- Red curve indicates trend of temperature
- Green curve indicates trend of humidity.
- Yellow curve indicates trend of noise.
- Ordinate scale indicates the value of temperature, humidity and noise.
- Abscissa indicates the date and time.
- The value of a certain point in time. (There will be a yellow line if you touch the area of curve and you can move it by click the "Last/Next" icon << >>).

## Digital Area (Timeout Screen)

- 1. "Temperature" indicates value of Temperature.
- 2. "Humidity" indicates value of Humidity.
- 3. "Noise" indicates value of Noise.
- 4. If an alarm occurs, an alarm icon will appear.



## Menu

Click Menu Button in main interface to come into below interface, can set various parameters and view version information etc.

The image shows a menu screen with a list of options on the left and a settings panel on the right. The options are: General setup, Recording setup, View Alarms, History, Display, Date & Time, and Info. The settings panel includes: Temperature Unit (°F selected), Alarm (On), Beeper (On), A/C (On), F/S (On), Temperature Alarm (High and Low), Humidity Alarm (High and Low), Noise (High), and a Save button.

| Option            | Value                              |
|-------------------|------------------------------------|
| Temperature Unit  | °F                                 |
| Alarm             | On                                 |
| Beeper            | On                                 |
| A/C               | On                                 |
| F/S               | On                                 |
| Temperature Alarm | High Alarm: _____ Low Alarm: _____ |
| Humidity Alarm    | High Alarm: _____ Low Alarm: _____ |
| Noise             | High Alarm: _____                  |

## General Setup

Set parameter of temperature units and alarm value of Temperature/Humidity/Noise.



1. Temperature Unit: switch to units °C/°F.

2. Alarm: check the box to set alarm value of the temperature, humidity and noise. 3. Click “Save” to save setting parameter.

Note: After save the alarm value, if the alarm is triggered, the lamp will light up and send beeps,


such as box shown in the pictures below:



## Recording Setup

Set recording sampling rate and total number of samples.



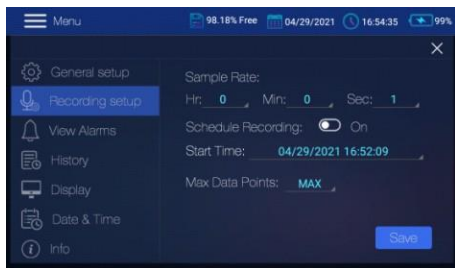

1. Sample Rate: Set recording rate, the minimum is 1s.
2. Schedule recording: The recording will start automatically when the set time comes.
3. Max data points: Set total record points.

## Alarms

View recorded alarm value.





1. Sort by date: View recorded alarm value by date sorting.
2. Sort by value: View recorded alarm value of noise, Temperature and Humidity.

## History

- Review history data: Select "All" and click "Delete", it will delete all history files.

- Click history recorded files, and pop Open/Delete option, select anyone and “Delete”, it will delete the history file that you select.

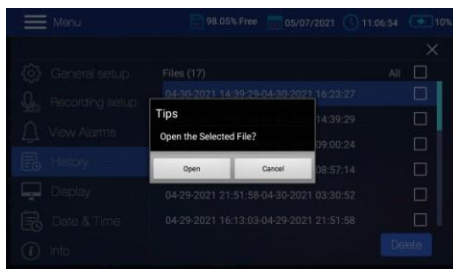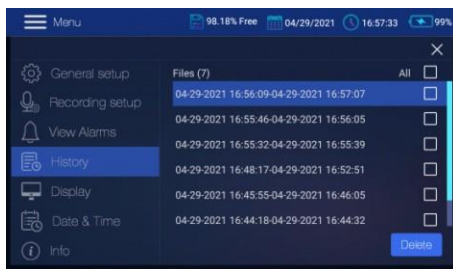

- If select Open, it will jump to the history recorded interface, as follows



- CSV Files: CSV file is generated automatically , and could be reviewed after connected to the computer, the method of the csv files import into the computer:

1.Connect the instrument to the computer via USB cable, and “Datalogger” will appear on the computer.


2.Click “Datalogger” to open “USB storage”, CSV files are stored in the rh-t data folder.

3.Open any CSV file to view the Temperature, Humidity and Noise data recorded in the instrument history (Note: CSV file is similar to Excel file, computer itself needs to install such tools).

|    | A   | B          | C    | D         | E          | F        | G |
|----|-----|------------|------|-----------|------------|----------|---|
| 1  | NO. | Temp (Fahr | CO2  | Dew point | Time       |          |   |
| 2  | 1   | 71.2       | 6000 | 57.7      | 01/01/2015 | 06:41:30 |   |
| 3  | 2   | 71.2       | 6000 | 57.7      | 01/01/2015 | 06:41:31 |   |
| 4  | 3   | 71.2       | 5890 | 57        | 01/01/2015 | 06:41:32 |   |
| 5  | 4   | 71.2       | 5800 | 56.8      | 01/01/2015 | 06:41:33 |   |
| 6  | 5   | 71.2       | 5700 | 57.4      | 01/01/2015 | 06:41:34 |   |
| 7  | 6   | 71.2       | 5700 | 58.6      | 01/01/2015 | 06:41:35 |   |
| 8  | 7   | 71.2       | 5690 | 57.9      | 01/01/2015 | 06:41:36 |   |
| 9  | 8   | 71.2       | 5680 | 57.9      | 01/01/2015 | 06:41:37 |   |
| 10 | 9   | 71.2       | 5670 | 57.7      | 01/01/2015 | 06:41:38 |   |
| 11 | 10  | 71.2       | 5660 | 57.2      | 01/01/2015 | 06:41:39 |   |
| 12 | 11  | 71.2       | 5500 | 56.5      | 01/01/2015 | 06:41:40 |   |
| 13 | 12  | 71.2       | 5400 | 55.9      | 01/01/2015 | 06:41:41 |   |

## Display

Adjust the brightness of screen.

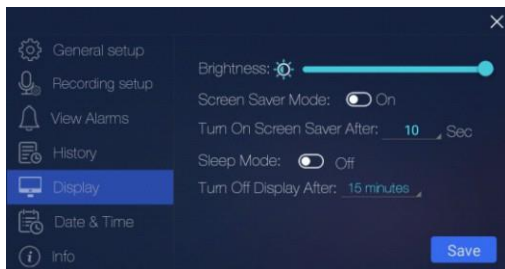


1.Brightness: Drag Brightness button to adjust brightness of screen.

2.Screen saver: Set the automatic screen saver time, active only after turn on the screen saver mode. 3.Sleep Mode: Set starting time of screensaver: 15 minutes, 30 minutes, 4 hours, 12 hours and


Never, active only after turn on the sleep mode. 4.Click “Save” to save setting parameter.

## Date & Time

- Click the area of time to set date and time.
- Choose Date format.
- As fellows:

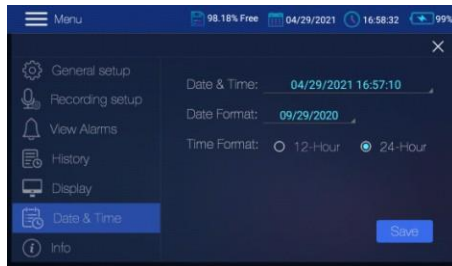


- Setup the time and click the “YES” will modify the system time.

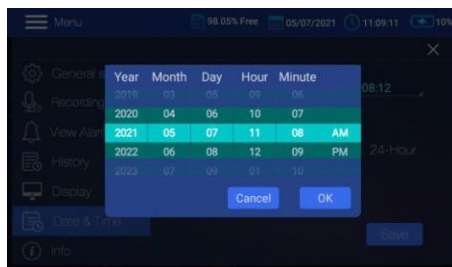

## Info

View instrument information and upgrade.

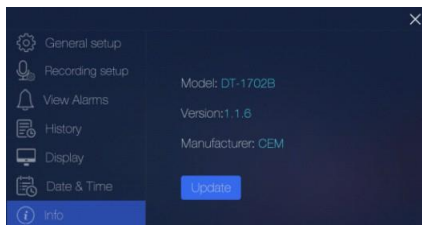

1.Version: Current versions.

2.Update: Click the button to update software.

Note: The upgrading app is follows:

- The instrument is connected to the computer via a USB cable.
- Find out in hard drive of the instrument in the computer, and then copy the latest APP to the download directory of the instrument.
- Click “Update” to realize upgrade.

## Exit Menu

Click this button to return to main UI.

- If necessary, use wet cloth and non-irritating detergent to clean the equipment and wipe the machine case.
- Do not use corrosive or irritating cleaners.
- Clean the display with a dry, smooth cloth.
- Do not immerse the product in water or other liquids.

## ***Specifications***

---

|                     |  |
|---------------------|--|
| Temperature         | -4 to 176°F (-20 to 80°C)  |
| Accuracy            | Accuracy : $\pm 0.5^{\circ}\text{C}/0.9^{\circ}\text{F}$ at -10 to 40°C/14 to 104°F (For Tablet)<br>$\pm 1.5^{\circ}\text{C}/3.0^{\circ}\text{F}$ at -20 to -10°C/-4 to 14°F (For Sensor Prob)<br>$\pm 0.5^{\circ}\text{C}/0.9^{\circ}\text{F}$ at -10 to 80°C/14 to 176°F (For Sensor Prob) |
| Relative Humidity   | 10 to 95%RH  |
| Accuracy            | Accuracy : $\pm 2.5\%\text{RH}$ at 20% to 80%RH<br>$\pm 3.0\%\text{RH}$ at 10% to 20%RH/80% to 95%RH   |
| Sound Level         | 30 to 130dB  |
| Accuracy            | $\pm 1.4\text{dB}$ (1kHz)  |
| Frequency Range     | 31.5Hz to 8kHz   |
| Frequency Weighting | A and C  |
| Response Time       | Fast (125ms) and Slow (1s)   |
| Resolution          | 0.1°F/°C; 0.1%RH/0.1dB   |
| Memory              | 16GB   |
| Datalogging Points  | 20,000 points total  |
| Sampling Intervals  | 1sec to 24hr   |
| PC Interface        | USB  |
| Power               | 3.7V Lithium Battery/5V 2A AC Adapter  |
| Dimensions          | 7.1 x 4.5 x 0.7" (180 x 115 x 18mm)  |
| Weight              | 1lbs (450g)  |

## ***Warranty***

---

Triplett / Jewell Instruments extends the following warranty to the original purchaser of these goods for use. Triplett warrants to the original purchaser for use that the products sold by it will be free from defects in workmanship and material for a period of (1) one year from the date of purchase. This warranty does not apply to any of our products which have been repaired or altered by unauthorized persons in any way or purchased from unauthorized distributors so as, in our sole judgment, to injure their stability or reliability, or which have been subject to misuse, abuse, misapplication, negligence, accident or which have had the serial numbers altered, defaced, or removed. Accessories, including batteries are not covered by this warranty

**Copyright © 2022 Triplett**

**[www.triplett.com](http://www.triplett.com)**



SE



NO

**Direktronik AB** | Box 234, 149 23 Nynäshamn | Besöksadress Konsul Johnsons väg 15 149 45 Nynäshamn

Telefon 08 52 400 700 | Fax | Epost [info@direktronik.se](mailto:info@direktronik.se) | Org.nr 556281-9663 | Bankgiro 922-0179